



Cervical Plan - EMG

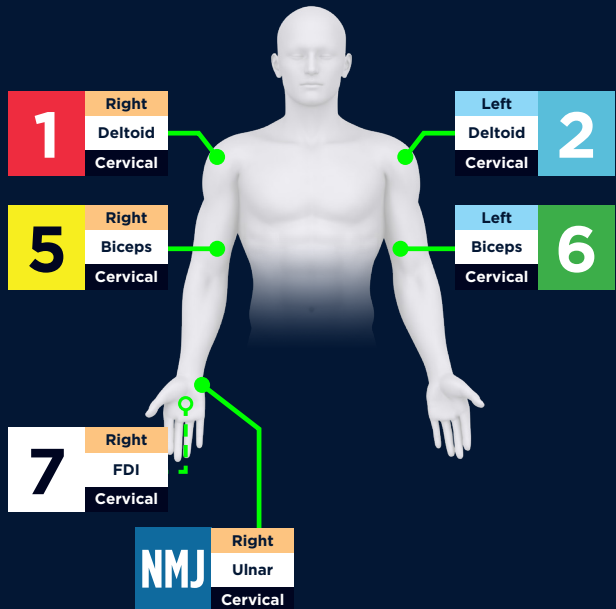

SafeOp™

NEURAL INFORMATIX SYSTEM

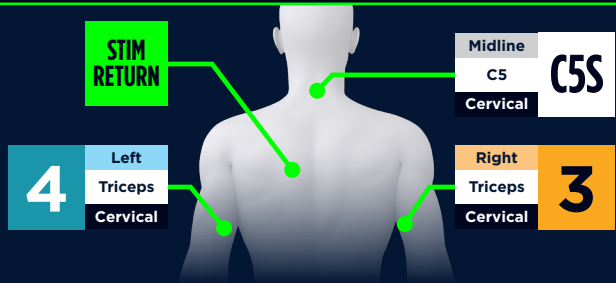

SafeOp™

NEURAL INFORMATIX SYSTEM

ALPHATEC SPINE, THE ATEC LOGO, SAFEOP, AND ALPHAINFORMATIX ARE TRADEMARKS OR REGISTERED TRADEMARKS OF ALPHATEC HOLDINGS, INC., ITS AFFILIATES AND/OR SUBSIDIARY COMPANIES.

© 2019 ALPHATEC SPINE, INC. ALL RIGHTS RESERVED.
LIT-84892A | 2019/10/18

EMG Quickstart Guide

atec™

CORPORATE HEADQUARTERS
5818 EL CAMINO REAL
CARLSBAD, CA 92008

CUSTOMER SERVICE
TOLL FREE: 800.922.1356
LOCAL: 760.431.9286
FAX: 800.431.1624

atec™
Spine Approach Technologies

AlphaInformatix™

1

WAITING FOR HEAD UNIT

Confirm that Wi-Fi is enabled on the tablet and Head Unit is powered on. Use the supplied SafeOp Data Cable if the issue persists.

2

RED ELECTRODE OR EMG NOISE

Check electrode connection to both the patient and the harness, and replace if necessary.

3

LOW/NO AUDIO

Press "+" button on tablet to increase volume. Confirm audio is enabled (🔊) on the SafeOp application.

4

CHECK PROBE MESSAGE

Confirm that Stim Return electrode is in contact with the patient and connected to the Head Unit. Confirm that the Clip or Probe is connected to the Head Unit and is in contact with the patient.

5

ERROR CODE ##

Press "OK" to clear message. If issue persists, turn the Head Unit off and back on. Close the SafeOp app by pressing the Square button and swiping left on the SafeOp app's window. Reopen the SafeOp app and select "Resume Case."

SafeOp Support Hotline:

844.SafeOp1 / 844.723.3671

